

[Type text]

THERMAL INSTRUMENT Co.

217 Sterner Mill Road, Treose, PA 19053

Telephone No. (215) 355-8400

FAX No. (215) 355-1789

Email: office@thermalinstrument.com

Hot Tapping Options

For

Flow Meter 62-9

MODEL:

62-9


220VAC

110VAC

24 VDC

Factory Set

[Type text]

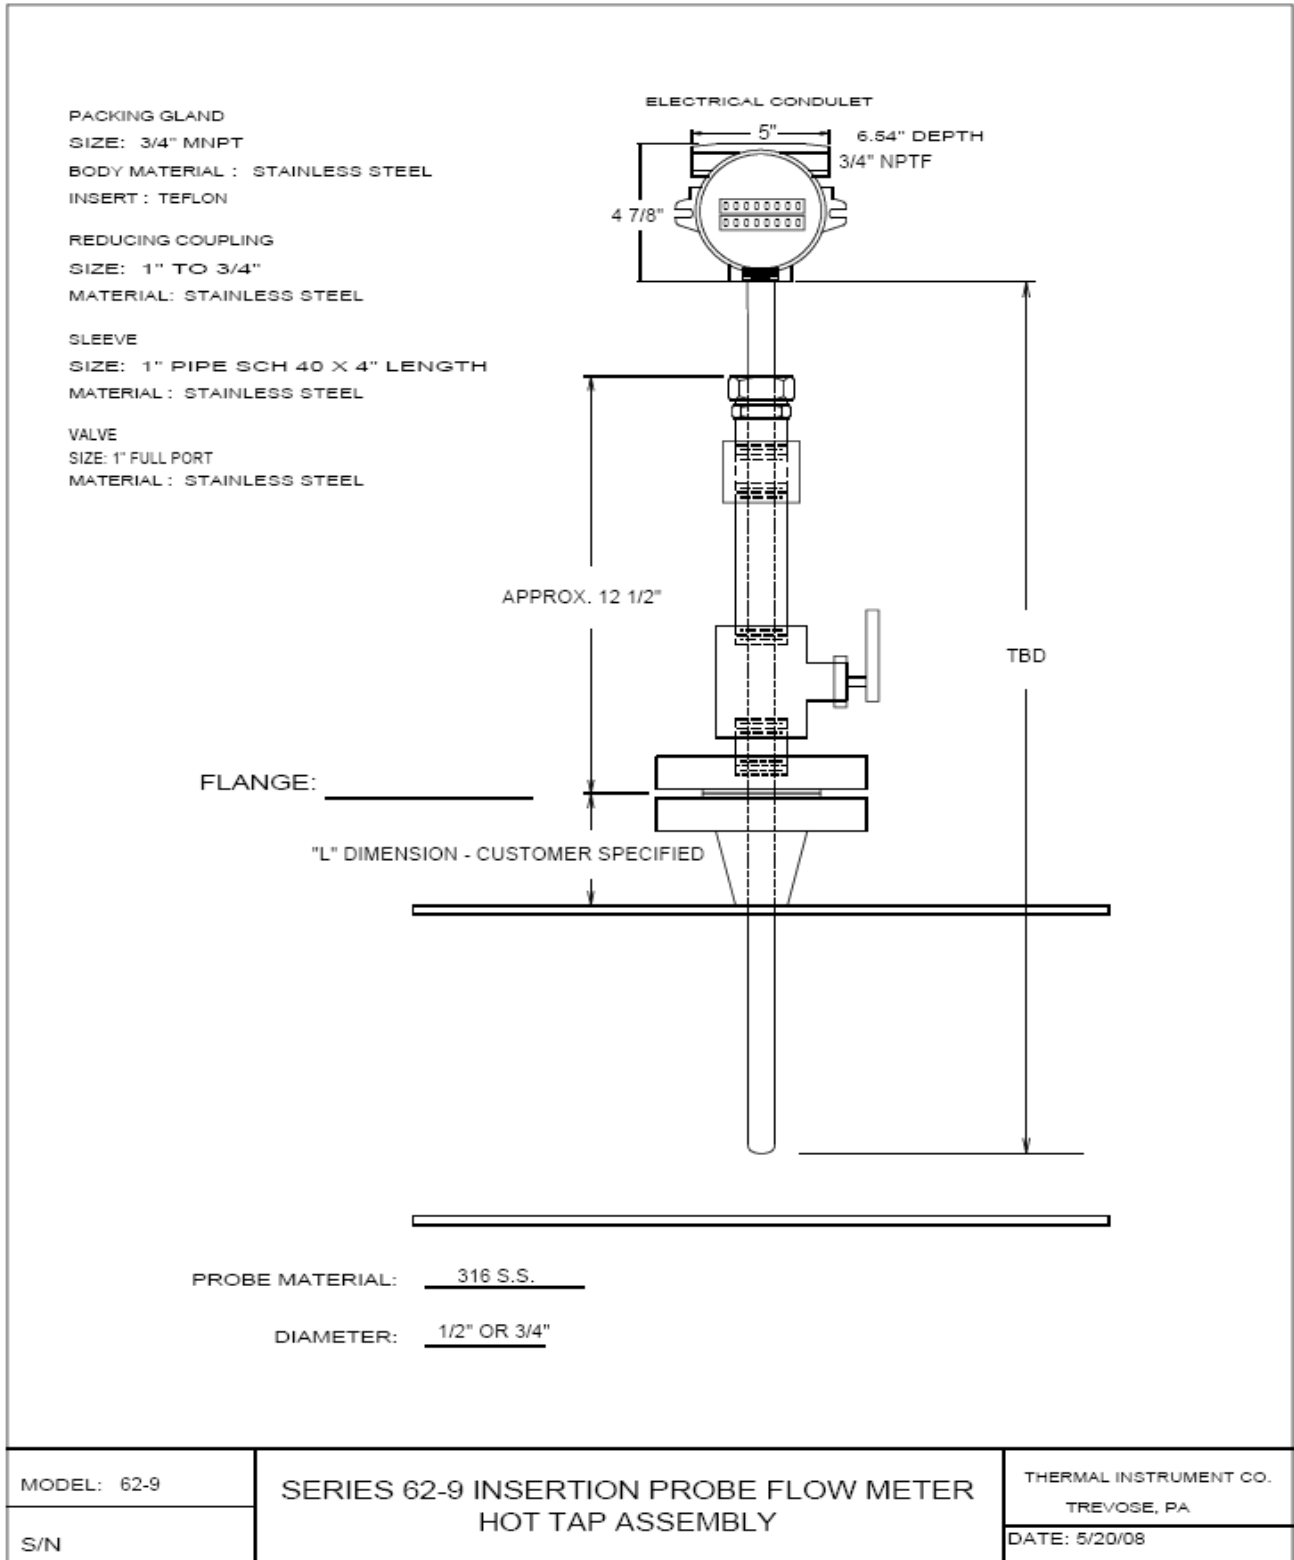

[Type text]

PACKING GLAND
SIZE: 3/4" MNPT
BODY MATERIAL : STAINLESS STEEL
INSERT : TEFLON


REDUCING COUPLING
SIZE: 1" TO 3/4"
MATERIAL: STAINLESS STEEL

SLEEVE
SIZE: 1" PIPE SCH 40 X 4" LENGTH
MATERIAL : STAINLESS STEEL

VALVE
SIZE: 1" FULL PORT
MATERIAL : STAINLESS STEEL

THREAD-O-LET
(ALSO KNOWN AS PIPE SADDLE)

PLEASE CONTACT THERMAL INSTRUMENT CO.
IF ANY OTHER CONNECTION CONFIGURATION
IS USED, AS THIS MAY BE CRITICAL IN DETERMINING
PROBE LENGTH.

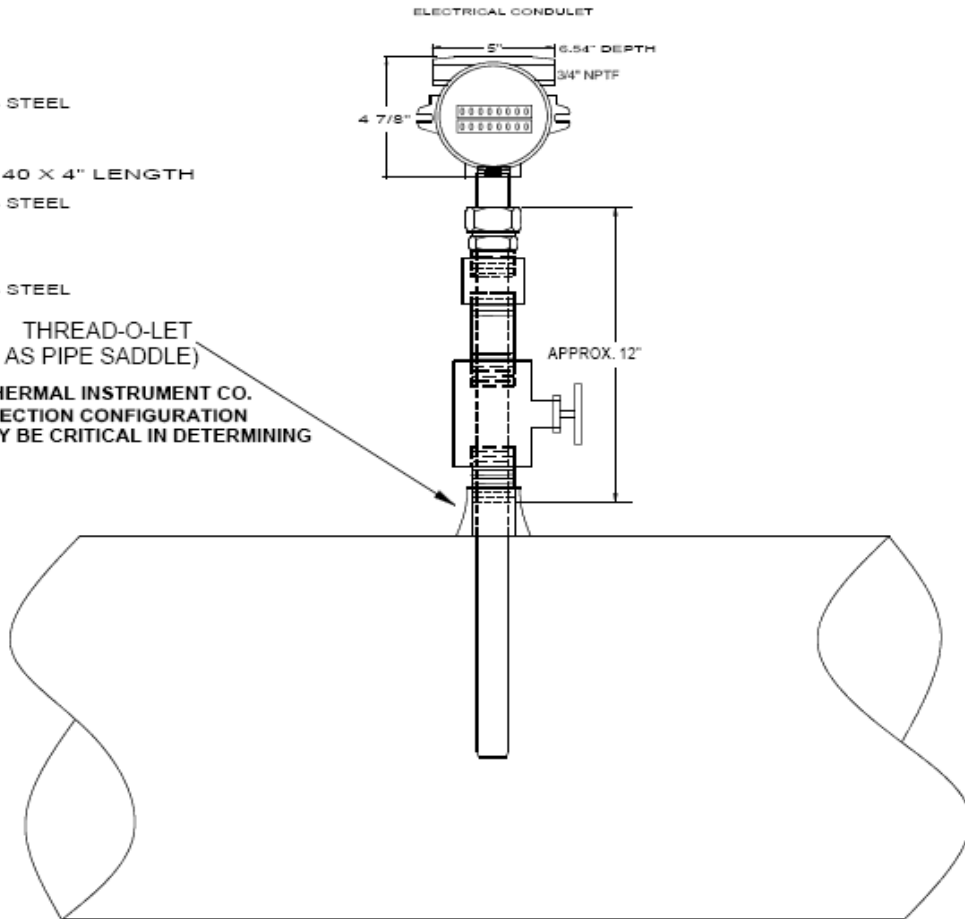

PROBE:

TOTAL LENGTH: TBD

DIAMETER: 1/2" or 3/4"




MATERIAL: 316 S.S.

MODEL: 62-9	INSTALLATION OF MODEL 62 PROBE WITH HOT TAPPING ASSEMBLY WITH THREADED CONNECTIONS	THERMAL INSTRUMENT COMPANY TREVOSE, PA
S/N		DATE: 5/20/08


[Type text]


Material:
 HALF COUPLING CARBON STEEL
 PLATE CARBON STEEL
 PIPE NIPPLES 304 SS
 BALL VALVE STAINLESS STEEL
 PACKING GLAND STAINLESS STEEL
 PROBE STAINLESS STEEL

PROBE DIAMETER: 3/4" O.D.
 PROBE LENGTH: TBD

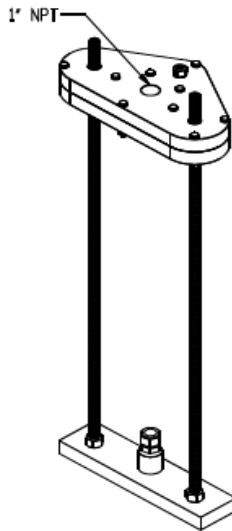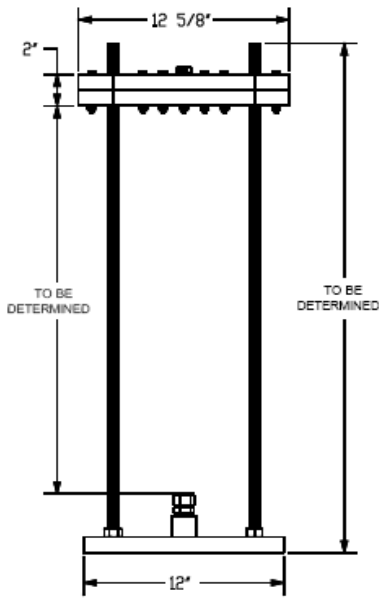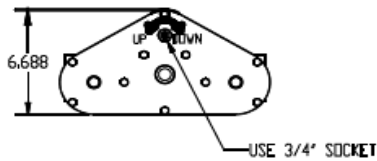

RETRACTOR ASSEMBLY

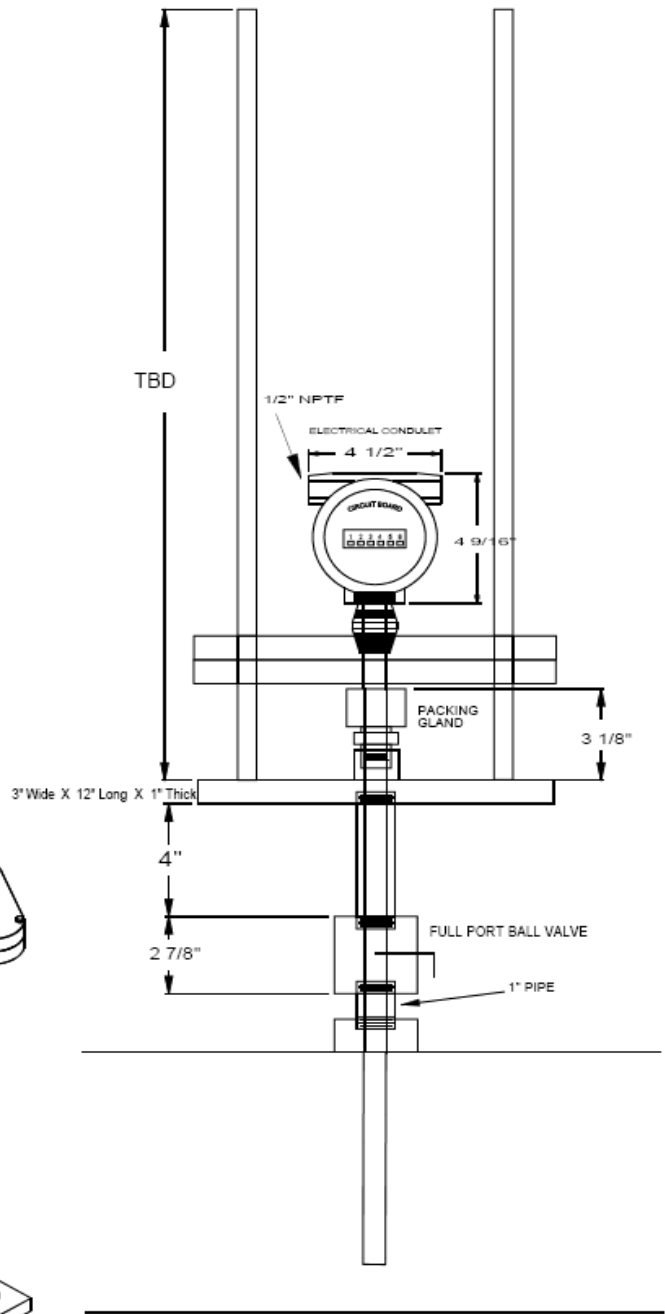

SERIAL NO.	 Thermal Instrument Company 217 Sterner Mill Road, Treveose, PA 19053, USA		
	DWG NO: RETRACTS.DC2	DESCRIPTION: PROBE TYPE FLOW METER WITH RETRACTOR	
<small>Thermal Instrument Company Proprietary Statement: This drawing is the property of Thermal Instrument Company. Unauthorized use of this document is prohibited and subject to enforcement if violated.</small>	ORIGINATION DATE: 12/22/06	DRAWN BY: MJH	APPROVED BY: MJH
SCALE: NONE	MATERIAL: AS NOTED	PAGE: 1 of 1	

[Type text]

